



LABORATORY RESULTS – KODIAKCOOLER® WHITE PAPER

**Biodegradation Test by Independent Lab
KODIAKOTTON® Wrapped and Unwrapped**




BIODEGRADATION STUDY on KODIAKOTTON®

Conducted by Biosystems Atlanta, A Unit of Biosystems America, Biosystems, Inc.

Test protocol: AOAC, APHA, ASTM, Bio-SOP, EPA, FDA-BAM, USDA, Vendor-SOP, Other (Specify): DD5511

Material Specs: KODIAKOTTON® 100% Non-Wo

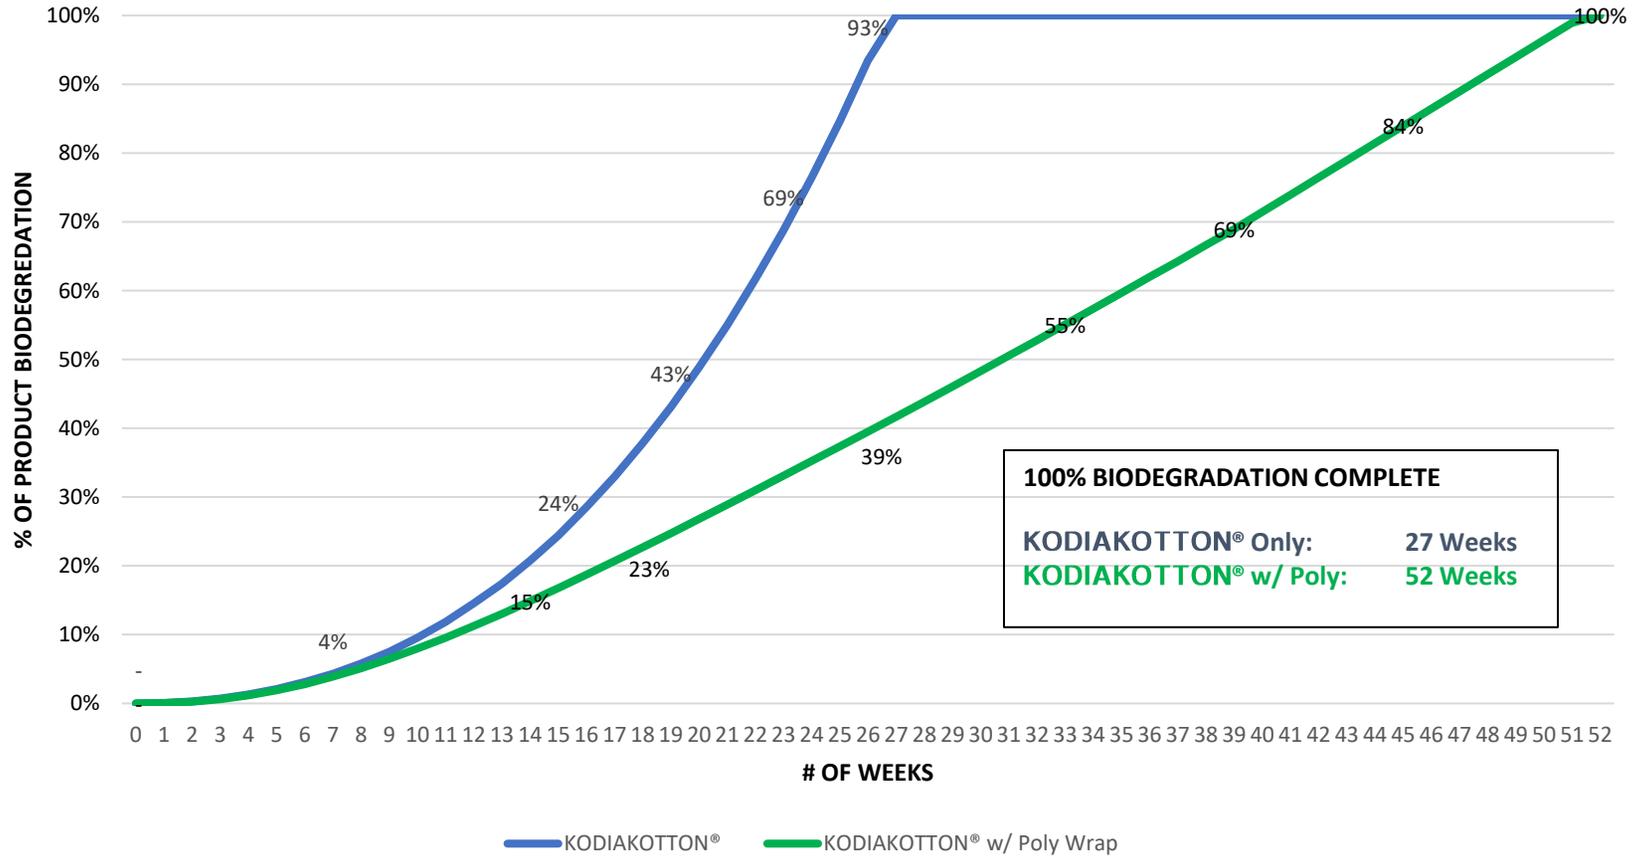

The above test results were conducted by a certified, independent laboratory and includes, but is not limited to certain limitations such as "Without any conflict of interest, we unconditionally guarantee the confidentiality of this agreement and the quality of the work performed, but make no representations re: fitness of the results for any particular purpose, unless so stated in a specific Letter of Professional Opinion rendered by us or so stated in Results." KODIAKOTTON® provides this information as guidance only and does not warrant or guarantee these results for any particular application. Copies of the entire laboratory analysis report are available upon request. © 2017 KODIAKOTTON®